


**N4L Newtons4th Ltd**

PPA5500

KinetiQ

COMMUNICATIONS MANUAL

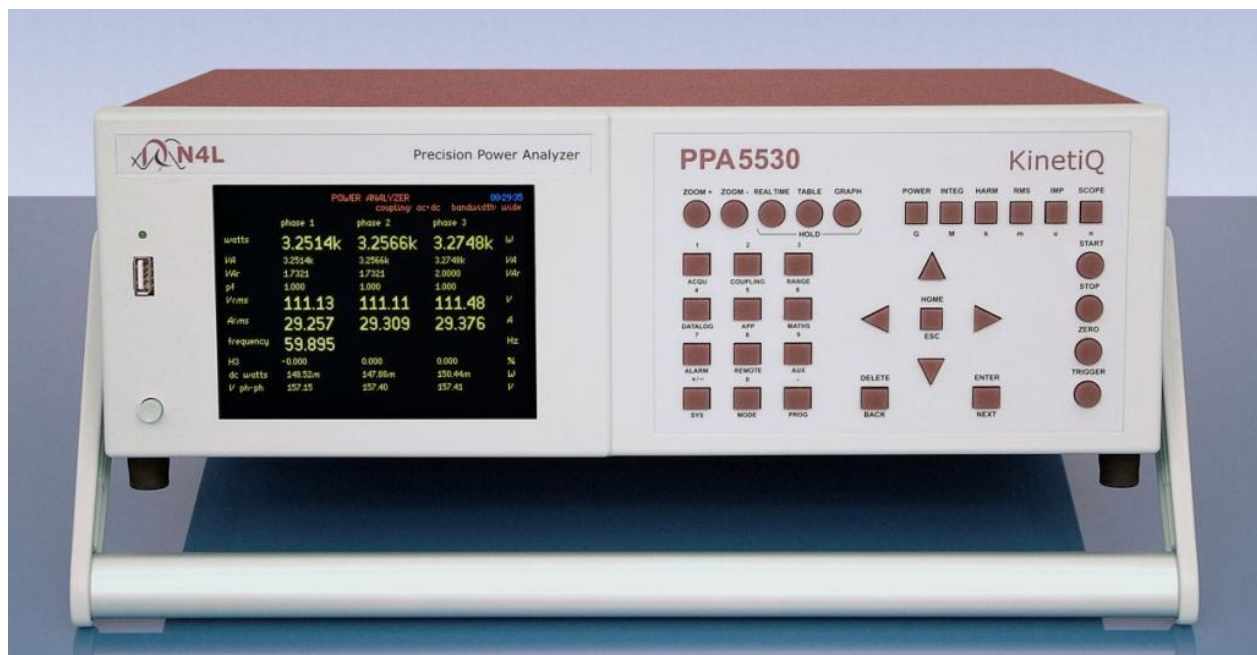

IMPORTANT SAFETY INSTRUCTIONS

This equipment is designed to comply with BSEN 61010-1 (2001) (Safety requirements for electrical equipment for measurement, control, and laboratory use) – observe the following precautions:

- Ensure that the supply voltage agrees with the rating of the instrument printed on the back panel **before** connecting the mains cord to the supply.
- This appliance **must** be earthed. Ensure that the instrument is powered from a properly grounded supply.
- The inputs are rated at 1kV rms or dc cat II; 600V rms or dc cat III. **Do not exceed the rated input.**
- Keep the ventilation holes on the underneath and rear free from obstruction.
- Do not operate or store under conditions where condensation may occur or where conducting debris may enter the case.
- There are no user serviceable parts inside the instrument – do not attempt to open the instrument, refer service to the manufacturer or his appointed agent.

Note: Newtons4th Ltd. shall not be liable for any consequential damages, losses, costs or expenses arising from the use or misuse of this product however caused.

ABOUT THIS MANUAL

This manual gives details of the communication commands recognized by the PPA55xx series of instruments over RS232, USB, LAN or GPIB. For more general operating instructions for the instrument refer to the specific user manual.

Each command is listed alphabetically with details of any arguments and reply. A one line summary of each command is given in the appendix. Although most of the commands apply to all instruments in the range there are some commands that are specific to one instrument or another.

The information in this manual is believed to be accurate and complete but Newtons4th Ltd cannot accept any liability whatsoever for any consequential damage or losses arising from any errors, inaccuracies, or omissions.

Revision 2.64

This manual is copyright © 2006-2014 Newtons4th Ltd. and all rights are reserved. No part may be copied or reproduced in any form without prior written consent.

02nd July 2014

CONTENTS

1	Using remote control	1-1
1.1	Standard event status register.....	1-3
1.2	Serial Poll status byte	1-4
1.3	RS232 connections.....	1-5
1.4	Data format	1-6
2	Communication commands	2-1
	*CLS	2-1
	*ESE	2-2
	*ESR?.....	2-3
	*IDN?.....	2-4
	*OPC?	2-5
	*RST	2-6
	*SRE	2-7
	*SRE?.....	2-8
	*STB?.....	2-9
	*TRG	2-10
	*TST?.....	2-11
	*WAI	2-12
	ABORT	2-13
	ALARM	2-14
	ALARM?	2-15
	ALARM1	2-16
	ALARM2	2-17
	ALARME	2-18
	ALARME?.....	2-19
	APPLIC.....	2-20
	BANDWI	2-21
	BANDWI?	2-22
	BEEP	2-23
	BLANKI	2-24
	CALVER	2-25
	CALVER?	2-26
	CAPTUR?.....	2-27
	CONFIG	2-29
	CONFIG?.....	2-30
	COUPLI	2-31
	COUPLI?	2-32
	DATALO	2-33
	DATALO?.....	2-34

PPA55xx communications manual

DAV?	2-35
DAVER	2-36
DAVER?	2-37
DISPLAY	2-38
DISPLAY?	2-39
EFFICI	2-40
EFFICI?	2-41
FAST	2-42
FQLOCK	2-43
FQREF	2-44
FREQFI	2-45
FREQUE	2-46
FSD?	2-47
Function:	2-47
HARMON	2-48
HARMON?	2-49
HOLD	2-50
INPUT	2-51
INTEGR	2-52
INTEGR?	2-53
KEYBOA	2-54
LCR	2-55
LCR?	2-56
LOWFRE	2-57
MODE	2-58
MSLAVE	2-59
MULTIL	2-60
MULTIL?	2-61
NEWLOC	2-62
NOISEF	2-63
NOOVER	2-64
PFCNV	2-65
PHASEM	2-66
PHASEM?	2-67
PHCONV	2-68
POWER	2-69
POWER?	2-70
PROGRA	2-72
PROGRA?	2-73
RANGE	2-74
RESOLU	2-75
RESULT	2-76
RESULT?	2-77
REZERO	2-78

PPA55xx communications manual

SCALE	2-79
SCOPE?	2-80
SCREEN?.....	2-81
SETUP	2-82
SETUP?	2-83
SHUNT.....	2-84
SMOOTH	2-85
SPEED	2-86
START	2-87
STATUS?.....	2-88
STOP	2-89
SUSPEN	2-90
TAGREP	2-91
TEMPER	2-92
TEMPER?.....	2-93
TORQSP.....	2-94
TORQSP?	2-95
USER?	2-96
VARCON	2-97
VERSIO?	2-98
VRMS	2-99
VRMS?	2-100
WIRING	2-101
ZERO.....	2-102
ZOOM.....	2-103
ZOOM?	2-104
 Multilog Application Guide.....	 2-105

Appendix A – command summary

Appendix B – configurable parameters

Appendix C – MULTILOG parameters

1 Using remote control

The instrument is fitted with an RS232 serial communications port, USB, IEEE488 (GPIB) and LAN interface. All the interfaces use the same ASCII protocol with the exception of the end of line terminators:

	Rx expects	Tx sends
RS232 USB, LAN	carriage return (line feed ignored)	carriage return and line feed
IEEE488	carriage return or line feed or EOI	carriage return with EOI

All the functions of the instrument can be programmed via any interface, and results read back. When the IEEE488 interface is set to 'remote' the other ports are ignored.

The commands are not case sensitive and white space characters are ignored (e.g. tabs and spaces). Replies from the instrument are always upper case, delimited by commas, without spaces.

Only the first six characters of any command are important – any further characters will be ignored. For example, the command to set the generator frequency is FREQUE but the full word FREQUENCY may be sent as the redundant NCY at the end will be ignored.

Fields within a command are delimited by comma, multiple commands can be sent on one line delimited with a semi-colon. Eg.

FQREF,CURRENT;POWER?

Mandatory commands specified in the IEEE488.2 protocol have been implemented, (e.g. *IDN?, *RST) and all commands that expect a reply are terminated with a question mark (query).

The instrument maintains an error status byte consistent with the requirements of the IEEE488.2 protocol (called the standard event status register) that can be read by the mandatory command *ESR? (See section 2).

The instrument also maintains a status byte consistent with the requirements of the IEEE488.2 protocol, that can be read either with the IEEE488 serial poll function or by the mandatory command *STB? over RS232 or IEEE or LAN (see section 2).

The IEEE address defaults to 23 and can be changed via the COMMS menu.

The keyboard is disabled when the instrument is set to "remote" using the IEEE. Press HOME to return to "local" operation.

RS232 data format is: start bit, 8 data bits (no parity), 1 stop bit. Flow control is RTS/CTS (see section 1.3), baud rate is selectable via the MONITOR menu.

A summary of the available commands is given in the Appendix. Details of each command are given in the communication command section of the manual.

Commands are executed in sequence except for two special characters that are immediately obeyed:

- Control T (20) – reset interface (device clear)
- Control U (21) – warm restart

1.1 Standard event status register

PON		CME	EXE	DDE	QYE		OPC
-----	--	-----	-----	-----	-----	--	-----

- bit 0 OPC (operation complete)
cleared by most commands
set when data available or sweep complete
- bit 2 QYE (unterminated query error)
set if no message ready when data read
- bit 3 DDE (device dependent error)
set when the instrument has an error
- bit 4 EXE (execution error)
set when the command cannot be executed
- bit 5 CME (command interpretation error)
set when a command has not been recognised
- bit 7 PON (power on event)
set when power first applied or unit has reset

The bits in the standard event status register except for OPC are set by the relevant event and cleared by specific command (*ESR?, *CLS, *RST). OPC is also cleared by most commands that change any part of the configuration of the instrument (such as MODE or START).

1.2 Serial Poll status byte

		ESB	MAV	ALA			RDV
--	--	-----	-----	-----	--	--	-----

- bit 0 RDV (result data available)
set when results are available to be read as enabled by DAVER
- bit 3 ALA (alarm active)
set when an alarm is active and enabled by ALARMER
- bit 4 MAV (message available)
set when a message reply is waiting to be read
- bit 5 ESB (standard event summary bit)
set if any bit in the standard event status register is set as well as the corresponding bit in the standard event status enable register (set by *ESE).

1.3 RS232 connections

The RS232 port on the instrument uses the same pinout as a standard 9 pin serial port on a PC or laptop (9-pin male 'D' type).

Pin	Function	Direction
1	DCD	in (+ weak pull up)
2	RX data	in
3	TX data	out
4	DTR	out
5	GND	
6	DSR	not used
7	RTS	out
8	CTS	in
9	RI	not used

The instrument will only transmit when CTS (pin 8) is asserted, and can only receive if DCD (pin 1) is asserted. The instrument constantly asserts (+12V) DTR (pin 4) so this pin can be connected to any unwanted modem control inputs to force operation without handshaking. The instrument has a weak pull up on pin 1 as many null modem cables leave it open circuit. In electrically noisy environments, this pin should be driven or connected to pin 4.

To connect the instrument to a PC, use a 9 pin female to 9 pin female null modem cable:

1 & 6	-	4
2	-	3
3	-	2
4	-	1 & 6
5	-	5
7	-	8

1.4 Data format

Non integer results are sent as ASCII characters in a scientific format consisting of 5 or 6 digit mantissa plus exponent:

```
+1.2345+E00
+1.23456+E00
```

For higher speed transfer a proprietary binary format can be selected which compresses the data into 4 bytes, each of which is sent with the msb set to distinguish them from ASCII control characters. The data is sent as a 7 bit signed exponent, a mantissa sign, and a 20 bit mantissa:

byte	data
1	7 bit signed exponent +63 to -64
2	bit 6 = mantissa sign bit 5:0 = mantissa bit 19:14
3	mantissa bit 13:7
4	mantissa bit 6:0

The value is coded as a binary fraction between 0.5 and 0.9999..., a multiplier of 2^n and a sign ie:

$$\text{Value} = (\text{mantissa} / 2^{20}) \times 2^{\text{exponent}} \times -1^{\text{sign}}$$

value	equivalent	hex data transmitted
3.0	0.75×2^2	0x82,0xB0,0x80,0x80
0.1	0.8×2^{-3}	0xFD,0xB3,0x99,0xCD
-320	-0.625×2^9	0x89,0xE8,0x80,0x80

Any valid number would have the msb of the mantissa set; any number without the msb of the mantissa set is zero.

2 Communication commands

***CLS**

***CLS**

Function: Clear status

Description: Clears the *standard event status register*.

Format: *CLS

Arguments: none

Reply: none

Example: *CLS
*ESR?
0

Notes:

***ESE**

***ESE**

Function: Set standard event status enable register.

Description: Enable which bits of the *standard event status register* set the ESB bit in the serial poll status byte..

Format: *ESE, value

Arguments: decimal equivalent of bits in standard event status enable register

Reply: can be read by *ESE?

Example: *ESE, 60

Notes: The following bits in the standard event status enable register have been implemented:

- bit 0 OPC (operation complete)
- bit 2 QYE (unterminated query error)
- bit 3 DDE (device dependent error)
- bit 4 EXE (execution error)
- bit 5 CME (command interpretation error)
- bit 7 PON (power on event)

For example, *ESE, 60 enables all the error bits so that the ESB bit in the serial poll status byte is set in the event of any error.

***ESR?**

***ESR?**

Function: Standard event status register query

Description: Returns the contents of the *standard event status register* and clears it.

Format: *ESR?

Arguments: none

Reply: decimal equivalent of bits in standard event status register

Example: *ESR?
33

Notes: The following bits in the standard event status register have been implemented:

- bit 0 OPC (operation complete)
- bit 2 QYE (unterminated query error)
- bit 3 DDE (device dependent error)
- bit 4 EXE (execution error)
- bit 5 CME (command interpretation error)
- bit 7 PON (power on event)

For example, if a command is sent incorrectly and is not recognised, the CME bit will be set and the value of 33 will be returned.

***IDN?**

***IDN?**

Function: Identify query

Description: Returns a standard format identification string.

Format: *IDN?

Arguments: none

Reply: An ASCII string in the IEEE488.2 format:
manufacturer,model,serial no,version

Example: *IDN?
NEWTONS4TH,PPA2530 KinetiQ,
01234,1.00

Notes:

***OPC?**

***OPC?**

Function: Test for operation complete

Description: Returns 1 if previous operation is completed, 0 if not.

Format: *OPC?

Arguments: none

Reply: 0 or 1

Example: START
*OPC?
0
*OPC?
0
*OPC?
1

Notes: *OPC? can be used to indicate when data is available or when a frequency sweep has completed.

***RST**

***RST**

Function: Reset

Description: Resets the instrument to the default state and clears the *standard event status register*.

Format: *RST

Arguments: none

Reply: none

Example: *RST

Notes: The *RST command loads the default configuration. This is the same as loading the default configuration via the PROGRAM menu.

Any preceding setup commands will be overwritten.

***SRE**

***SRE**

Function: Set service request enable register.

Description: Enable which bits of the *status byte register* initiate a service request.

Format: *SRE, value

Arguments: decimal equivalent of bits in status byte register

Reply: can be read by *SRE?

Example: *SRE, 1
generate a service request when data available.

Notes:

***SRE?**

***SRE?**

Function: Read service request enable register.

Description: Read back the present setting of the service request enable register.

Format: *SRE?

Arguments:

Reply: decimal equivalent of bits in status byte register that would generate a service request.

Example: *SRE?
1

Notes:

***STB?**

***STB?**

Function: Read serial poll status byte

Description: Returns the decimal value of the serial poll status byte.

Format: *STB?

Arguments: none

Reply: decimal value of the serial poll status byte

Example: *STB?
1

Notes: The following bits in the serial poll status register have been implemented:

- bit 0 RDV (results data available)
- bit 3 ALA (alarm active)
- bit 4 MAV (message available)
- bit 5 ESB (standard event summary bit)

***TRG**

***TRG**

Function: Trigger

Description: Initiates a new measurement, resets the range and smoothing.

Format: *TRG

Arguments: none

Reply: none

Example: MODE,VRMS
*TRG
VRMS,SURG?

Notes:

***TST?**

***TST?**

Function: Self test query

Description: Returns the results of self test

Format: *TST?

Arguments: none

Reply: single integer
bit 0 – set if uncalibrated
bit 1 – set if error with analogue zero
> 15 – major system error

Example: *TST?
0

Notes:

***WAI**

***WAI**

Function: Wait for operation complete
Description: Suspends communication until the previous operation has completed
Format: *WAI
Arguments: none
Reply: none
Example: *TRG
*WAI
POWER,PHASE1?
Notes:

ABORT

ABORT

Function: Abort datalog
Description: Abort datalog data acquisition.
Format: ABORT
Arguments: none
Reply: none
Example: DATALOG, RAM, 0.02
START
wait for data values
ABORT

Notes:

ALARM

ALARM

Function: Set common controls for alarm1 and alarm2.

Description: Set the alarm latch and sounder control.

Format: *ALARM,latch,sounder*

Arguments: latch:
 ON
 OFF
 sounder:
 ENABLED
 DISABLED

Reply: none

Example: ALARM,ON,DISABLED

Notes:

ALARM?

ALARM?

Function: Read alarm status.

Description: Reads the status of the measurements and 2 alarms.

Format: ALARM?

Arguments: none

Reply: single integer
bit 0 data available
bit 1 data error
bit 2 alarm 1
bit 3 alarm 2

Example: ALARM?
1

Notes: An alarm is present if bit 0 is high (data is available) and either alarm 1 or alarm 2 bits are high.

ALARM1

ALARM1

Function: Set parameters for alarm1.
Description: Set alarm1 type and thresholds.
Format: *ALARM1,type,data,high,low*
Arguments: type:
 DISABLED
 HIGH
 LOW
 INSIDE
 OUTSIDE
 LINEAR
 data
 1-4
 high:
 high threshold
 low:
 low threshold
Reply: none
Example: *ALARM1,HIGH,1,2,0*
Notes: Both thresholds must be sent even if only one is used.

ALARM2

ALARM2

Function: Set parameters for alarm2.

Description: Set alarm2 type and thresholds.

Format: *ALARM2,type,data,high,low*

Arguments: type:
 DISABLED
 HIGH
 LOW
 INSIDE
 OUTSIDE
 data
 1-4 for zoom data
 high:
 high threshold
 low:
 low threshold

Reply: None

Example: *ALARM2,LOW,3,0,0.5*

Notes: Both thresholds must be sent even if only one is used.
There is no LINEAR option for alarm 2.

ALARME**ALARME**

Function: Set alarm status enable register

Description: Sets bits in the alarm status enable register to control which alarm bit if any set the alarm active bits in the status byte.

Format: *ALARME,value*

Arguments: decimal equivalent of alarm bits
 bit2 set bit 3 of status byte when
 alarm 1 is active
 bit3 set bit 3 of status byte when
 alarm 2 is active

Reply: none

Example: *ALARME, 12*
 **SRE,8*
 set bit 3 in status byte when either alarm
 1 or alarm 2 is active and generate a
 service request

Notes: default value is 0

ALARME?

ALARME?

Function: Read alarm status enable register

Description: Read back present bits in the alarm status enable register which controls the alarm active bit in the status byte.

Format: ALARME?

Arguments: none

Reply: decimal equivalent of alarm bits

Example: ALARME?
12

Notes:

APPLIC**APPLIC**

Function: Select application mode.

Description: Some applications require special settings within the instrument for optimum measurement

Format: *APPLIC,type,setting*

Arguments: type:
 NORMAL
 PWM
 BALLAST
 INRUSH
 POWERT
 STANDB
 setting:
 filter 0-2 (PWM only)
 0: 4kHz
 1: 1kHz
 2: 250Hz
 speed 0-3 (ballast only)
 0: fixed time
 1: fast
 2: medium
 3: slow

Reply: none

Example: *APPLIC,POWERT*
APPLIC,PWM,1

Notes:

BANDWI**BANDWI**

- Function: Select bandwidth.
- Description: The analogue bandwidth of the instrument can be selected as "wide" (to 3MHz). For low noise measurements at low frequency the bandwidth can be restricted to "low" (to 40kHz). For measurements of dc in the presence of large ac signal, the bandwidth can be further restricted to "dc only" (to 10Hz).
- Format: BANDWI,*phase,type*
- Arguments: phase:
 PHASE1
 PHASE2
 PHASE3
 type:
 WIDE
 LOW
 DCONLY
- Reply: none
- Example: BANDWI,WIDE
- Notes: Only use DCONLY to improve accuracy of measurement of small dc in the presence of a large ac signal. For normal dc measurements use bandwidth = LOW.

BANDWI?

BANDWI?

Function: Read bandwidth setting.

Description: Returns a numerical value for the bandwidth setting.

Format: BANDWI,*phase?*

Arguments: phase:
 PHASE1
 PHASE2
 PHASE3

Reply: 0 = WIDE
 1 = LOW
 2 = DONLY

Example: BANDWI,PHASE3,LOW
 BANDWI,PHASE3?
 1

Notes: If independent input control has not been enabled then the setting for phase 1 is used for all phases.

BEEP

BEEP

Function: Sound the buzzer

Description: Makes a "beep" from the instrument.

Format: BEEP

Arguments: none

Reply: none

Example: BEEP

Notes:

BLANKI

BLANKI

Function: Select blanking
Description: Enable or disable low value blanking.
Format: BLANKI,*value*
Arguments: value:
 ON
 OFF
Reply: none
Example: BLANKI,OFF
Notes:

CALVER**CALVER**

- Function: Load a calibration verification string.
- Description: When calibrated, the instrument stores a text string which can be read on the front panel (press SYS and LEFT). This shows the date of calibration. Users who subsequently verify the accuracy in their own calibration facilities can enter an alternative string with the new date. The original string is not overwritten but the alternative string is displayed instead.
- Format: *CALVER,string*
- Arguments: *string* is any sequence of printable alpha numeric characters. Use the underscore character to add a space between words. CALVER without a string argument clears the previously stored string.
- Reply: none
- Example: CALVER,12_DEC_2008_AMW
- Notes: As all white space is stripped from any communications string, the underscore character (ASCII 95 or 0x5F) must be used to space out the words. Underscore is shown as a space on the screen.

CALVER?

CALVER?

Function: Read back the calibration verification string.

Description: When calibrated, the instrument stores a text string which can be read on the front panel (press SYS and LEFT). This shows the date of calibration. Users who subsequently verify the accuracy in their own calibration facilities can enter an alternative string with the new date. The original string is not overwritten but the alternative string is displayed instead.

Format: CALVER?

Arguments: none.

Reply: alphanumeric string

Example: CALVER?
12_DEC_2008_AMW

CAPTUR?**CAPTUR?**

Function: Read back Capture mode data.

Description: Returns captured oscilloscope data. Data is returned in 200 lines of 250 values per channel.

Format: CAPTUR?

Arguments: none

Reply: Multiple data values.

Example: CAPTUR?

Notes: This command only applies to PPA5532 firmware. Capture mode operates as a sub function of the normal oscilloscope mode – When “capture mode” is enabled in the menu data is stored in a 50000 byte circular buffer per channel. Set the trigger mode to single shot and trigger as normal. Sending the CAPTUR? command reads this data.

Each line of data should return as follows:

```
[#3503] [h1][h2][d1.1][d1.2][d2.1] [2.2]
.....[d250.1][d250.2] [error] [CR] [LF]
```

Each line consists of:

- 5 bytes that represent #3503 (ASCII)
- 2 bytes that represent the Header bits including channel number [h1][h2]
- 500 bytes that represent the actual data.
- 250 pieces of data each made up of 2 bytes. d1.1 is data 1 bit 1, d1.2 is data 1 bit 2, d2.1 is data 2 bit 1, d2.2 is data 2 bit 2 etc.

PPA55xx communications manual

1 byte that represents the error checking bit [error].

1 byte that represents Carriage return [CR].

1 byte that represents Line Feed [LF]

Each 8 bit byte has the msb set in order to prevent any misinterpretation of data within drivers and software which otherwise could mistake data for carriage return etc. so 14 bit data values are returned.

CONFIG

CONFIG

Function: Direct access of configuration parameters

Description: Sets configuration parameter for which there may not be a direct command.

Format: *CONFIG,index,data*

Arguments: index is the number of the parameter
data is the data for that parameter

Reply: none

Example: CONFIG,6,1 (set phase convention)

Notes: The list of configurable parameters is given in the appendix.
CONFIG goes through the same limit checking as when entering data from the menus.

CONFIG?

CONFIG?

Function: Configurable parameter query

Description: Reads the present value of a single parameter.

Format: CONFIG,*index*?
or: CONFIG?*index*

Arguments: index is the parameter number

Reply: Value of parameter, real or integer as appropriate.

Example: CONFIG,6? (read phase convention)
0
CONFIG,6,1 (set phase convention)
CONFIG,6?
1

Notes: The list of configurable parameters is given in the appendix.

COUPLI

COUPLI

Function: Set ac or ac+dc coupling.

Description: Selects the input coupling for a given input channel.

Format: *COUPLI,phase,coupling*

Arguments: phase:
 PHASE1
 PHASE2
 PHASE3
 coupling:
 AC+DC
 ACONLY
 DCONLY

Reply: none

Example: COUPLI,PHASE2,AC+DC

Notes: In multi phase applications, the coupling on phase 1 is applied to other phases unless "independent input control" is enabled.

COUPLI?

COUPLI?

Function: Read ac/dc coupling setting.

Description: Returns a numerical value for the coupling setting.

Format: *COUPLI,phase,coupling*

Arguments: phase:
 PHASE1
 PHASE2
 PHASE3

Reply: 0 = AC+DC
 1 = AONLY
 2 = DONLY

Example: COUPLI,PHASE2,AC+DC
 COUPLI,PHASE2?
 0

Notes: In multi phase applications, the coupling on phase 1 is applied to other phases unless "independent input control" is enabled.

DATALO**DATALO**

Function:	Set up datalog
Description:	Sets datalog parameters or accesses datalog non-volatile store.
Format:	<i>DATALO,function,interval,speed</i>
Arguments:	function: DISABLE RAM NONVOL RECALL DELETE interval: datalog interval in seconds speed: HIGH
Reply:	none
Example:	DATALOG,NONVOL,10 DATALOG,RAM,0,HIGH
Notes:	set interval to 0 to record every measurement as fast as possible. Set HIGH to select high speed mode for any combination of W, VA, VAr, pf, Vrms, Arms, and frequency. If HIGH is not sent then high speed mode is reset.

DATALO?**DATALO?**

Function:	Read back datalog results
Description:	Return datalog values, one record per line, or the number of lines available
Format:	DATALO, <i>start,records?</i> DATALO,0? DATALO,LINES?
Arguments:	start: first record to return records: number of records to return 0: return all new records since last read
Reply:	3 to 6 data values depending on settings: index 1-n elapsed time in hours data1 data2 (if stored) data3 (if stored) data4 (if stored) one record per line
Example:	DATALOG,NONVOL,10 START wait for datalog STOP DATALOG,LINES? 30 DATALOG,21,3? 21,2.0000E-1,1.2345E0 22,2.1000E-1,5.6789E3 23,2.2000E-1,1.2345E0
Notes:	if no arguments are sent then DATALOG? returns all the available lines of data

DAV?

DAV?

Function: Data available query
 Description: Returns data availability status.
 Format: DAV?
 Arguments: none
 Reply: Decimal equivalent of data available bits:
 bit0 new data available
 bit1 data available
 bit2 harmonic series data available
 bit6 integration data available
 bit7 datalog data available

Example: SPEED,SLOW
 *TRG
 DAV?
 0
 DAV?
 0
 DAV?
 0
 DAV?
 3 (data available)

Notes: DAV? does not modify the status bits.

DAVER**DAVER**

Function: Set data available enable register

Description: Sets bits in the data available enable register to control which status bits set the data available bits in the status byte.

Format: *DAVER,value*

Arguments: decimal equivalent of data available bits
bit0 set bit 0 of status byte when new data available
bit1 set bit 0 of status byte when data available

Reply: none

Example: *DAVER, 1*
set bit 0 in status byte when new data is available

Notes: default value is 2:
bit 0 of status byte is set whenever data is available.

DAVER?

DAVER?

Function: Read data available enable register

Description: Read back present setting of the data available enable register, which controls the status bits that set the data available bits in the status byte.

Format: DAVER?

Arguments: none

Reply: decimal equivalent of bits

Example: DAVER?
4

Notes:

DISPLAY

DISPLAY

Function: Set the display page

Description: Selects the page on the display so that the zoom data can be used for alarms.

Format: DISPLAY,*page*

Arguments: page:
PHASE1
PHASE2
PHASE3
SUM
NEUTRAL
TOTAL
FUNDAMENTAL
VOLTAGE
CURRENT

Reply: None

Example: DISPLAY,FUNDAMENTAL

Notes: VOLTAGE is the same as TOTAL;
CURRENT is the same as FUNDAMENTAL.
They refer to the multiphase display modes.

DISPLAY?

DISPLAY?

Function: Read the displayed data

Description: Returns all the values presently on the screen.

Format: DISPLAY?

Arguments: none

Reply: Multiple floating point values separated by commas

Example: DISPLAY?

Notes:

EFFICI

EFFICI

Function: Set efficiency calculation

Description: Selects the data to be used for the efficiency calculation.

Format: *EFFICI,formula*

Arguments: formula:
0 – disabled
1 – phase 1 / phase 2
2 – phase 2 / phase 1
3 – slave / master
4 – master /slave
5 – mechanical sum
6 – sum / mechanical
7 – phase 3 / sum
8 – sum /phase

Reply: none

Example: EFFICIENCY,2

Notes:

EFFICI?

EFFICI?

Function: Read efficiency result

Description: Reads back the total and fundamental efficiency results.

Format: EFFICI?

Arguments: none

Reply: 2 data values separated by commas:
total, fundamental

Example: EFFICI?
data returned

Notes:

FAST

FAST

Function: Set fast communications mode.

Description: Disables the screen drawing for high speed operation.

Format: FAST,*value*

Arguments: value:
 ON
 OFF

Reply: none

Example: FAST,ON

Notes: FAST mode does not suppress the data acquisition which continues in the background. See SUSPEND to disable all non-communication functions.

FQLOCK

FQLOCK

Function: Lock frequency.

Description: Fix the frequency for analysis to the present value.

Format: FQLOCK,*value*

Arguments: value:
 ON
 OFF

Reply: none

Example: FQLOCK,ON

Notes: To fix the analysis to a specified frequency, first lock the frequency with FQLOCK,ON then send the desired frequency with the FREQUE command.

FQREF**FQREF**

Function:	Set frequency reference.
Description:	Select the channel to be used for measuring the frequency.
Format:	<i>FQREF,phase</i> <i>FQREF,channel</i> <i>FQREF,phase,channel</i>
Arguments:	channel: voltage current Speed Ac Line phase: PHASE1 PHASE2 PHASE3
Reply:	none
Example:	FQREF,CURRENT
Notes:	Measured phase is always referred to phase 1 voltage no matter what channel is selected to measure the frequency, unless phase 1 is not active (eg phase 2 only mode).

FREQFI

FREQFI

Function: Set the frequency filter

Description: Selects a filter to be applied to the data used for frequency measurement to help synchronise in noisy environments.

Format: FREQFI,*value*

Arguments: value:
ON
OFF

Reply: none

Example: FREQFI,ON

Notes: The filter is applied only to the data used for frequency measurement and does not change the data used for the measurements.

FREQUE**FREQUE**

Function:	Set the analysis frequency
Description:	Sets the analysis frequency in Hz for frequency lock mode.
Format:	FREQUE, <i>frequency</i>
Arguments:	frequency in Hz
Reply:	none
Example:	FQLOCK,ON FREQUE,5e4 (set frequency to 50kHz)
Notes:	Lock the frequency with FQLOCK,ON before sending the desired frequency with the FREQUE command.

FSD?**FSD?**

Function: Read the full scale of all input channels at once or that of an individually selected input channel.

Description: Returns the full scale value for all channels or that of a single selected channel.

Format: FSD?
FSD,CH?

Arguments: None
CH1, CH2, CH3, CH4, CH5, CH6

Reply: Up to six data values separated by commas

Example 1: FSD?
Data returned, data returned, data returned, data returned, data returned, data returned

Example 2: FSD,CH1?
Data returned

Notes: Number of channels that can be read and the number of data values returned is dependent on the number of phases selected in the instruments settings.
CH1 = PH1: Voltage Input
CH2 = PH1: Current Input
CH3 = PH2: Voltage Input
CH4 = PH2: Current Input
CH5 = PH3: Voltage Input
CH6 = PH3: Current Input

HARMON**HARMON**

Function: Set harmonic analyser mode.

Description: Set harmonic analyser mode and parameters.

Format: HARMON,*para,harmonic,max*

Arguments: para:
 THDD difference formula THD
 THDS harmonic series THD
 TIF Telephone Influence Factor
 THF Telephone Harmonic Factor
 TDD Total Demand Distortion
 TRD Total Rated Distortion
 HPHASE harmonic phase
 PH-PH Phase to Phase harmonics
 harmonic:
 individual harmonic for display
 max:
 length of harmonic series (to 100)

Reply: none

Example: HARMON,THDS,3,50

Notes: It is not necessary to send any arguments, but if any are sent they must be in the specified order. PH-PH command is reset by any THD command.

HARMON?**HARMON?**

Function: Harmonic analyser query

Description: Read harmonic results.
Sets harmonic analyser mode if not already set.
Waits for next unread data if necessary.
Clears new data available bit read by DAV?

Format: HARMON?
or: HARMON,*phase*?
or: HARMON,SERIES?
or: HARMON,*phase*,SERIES?

Arguments: phase:
PHASE1
PHASE2
PHASE3
NEUTRAL
PHASES

Reply: 11 data values separated by commas:
freq,mag1,mag2,hmag1,hmag2,h%1,
h%2,thd%1,thd%2,hphase1,hphase2
or: magnitude and percentage for each
harmonic, one channel per line
or: magnitude and phase for each harmonic,
one channel per line

Example: HARMON,PHASE2?
data returned

Notes: HARMON? waits for next unread data.

HOLD

HOLD

Function: Set data hold

Description: Turns data hold on or off. Useful for reading data from different phases without it being changed between reads.

Format: HOLD,state

Arguments: State:
ON
OFF

Reply: none

Example: HOLD,ON
POWER,PHASE1,WATTS?
POWER,PHASE2,WATTS?
POWER,PHASE3,WATTS?
HOLD,OFF

Notes:

INPUT**INPUT**

Function: Set input mode

Description: Selects the input type of the instrument

Format: *INPUT,channel,type*

Arguments: channel:
 CH1
 CH2
 type:
 INTERN
 EXTATT
 EXTSHU

Reply: none

Example: INPUT,CH1,EXTSHU

Notes: CH1 applies to all voltage channels
 CH2 applies to all current channels

INTEGR**INTEGR**

- Function: Set integrated power mode.
- Description: Set integrated power mode, whether the integration for Watts and current use signed or unsigned values, and whether accumulated or averaged values are computed.
Also sets up run time for integration over a specific interval.
- Format: *INTEGR,type,display*
INTEGR,RUNTIM,hours,minutes
- Arguments: type:
 SIGNED
 MAGNITUDE
display:
 TOTAL
 AVERAGE
hours:
 integer
minutes:
 integer
- Reply: none
- Example: INTEGR,MAGNITUDE,TOTAL
- Notes:

INTEGR?

INTEGR?

Function: Read integrated power mode.

Description: Read integrated power mode for the selected phase.

Format: `INTEGR,phase?`

Arguments: phase:
 PHASE1
 PHASE2
 PHASE3
 PHASES
 SUM

Reply: 13 values separated by commas
 time,Wh,WH.f,VAh,VAh.f,VArh,Varh.f
 pf,pf.f,V,V.f,Ah,Ah.f

Example: START
 wait for integration time
 INTEGR,PHASE1?
 data returned

Notes: INTEGR? without specifying the phase returns the appropriate single phase data.

KEYBOA

KEYBOA

Function: Disable front panel keyboard.

Description: The front panel keyboard can be disabled to prevent accidental operation.

Format: KEYBOARD,*value*

Arguments: value:
 ENABLE
 DISABLE

Reply: none

Example: KEYBOARD,DISABLE

Notes: The keyboard can be re-enabled from the front panel only by pressing the HOME key.

LCR

LCR

Function: Set LCR meter mode.
Description: Set LCR mode and conditions.
Format: LCR,*parameter*
Arguments: parameter:
 AUTO
 CAPACITANCE
 INDUCTANCE
 IMPEDANCE
Reply: none
Example: LCR,IMPEDA
Notes:

LCR?**LCR?**

Function:	LCR meter query
Description:	Read LCR meter results. Sets LCR meter mode if not already set. Waits for next unread data if necessary. Clears new data available bit read by DAV?
Format:	LCR, <i>phase?</i>
Arguments:	phase: PHASE1 PHASE2 PHASE3 PHASES
Reply:	11 data values separated by commas: freq, Vmag, Amag, impedance, phase, R, C, L, $\tan\delta$, Qf, reactance
Example:	LCR,IMPEDA LCR,PHASES? data returned
Notes:	LCR? waits for next unread data. LCR? without specifying the phase returns the appropriate single phase data.

LOWFRE

LOWFRE

Function: Set low frequency mode

Description: Sets the low frequency option for extending the measurement window.

Format: LOWFRE,*value*

Arguments: value:
ON
OFF

Reply: none

Example: LOWFRE,ON

Notes: LOWFRE is mainly used for measuring low frequencies (<5 Hz). However, as it applies digital filtering, it may also be useful when analysing any signals below a few hundred Hertz.

MODE**MODE**

Function: Set mode

Description: Sets the basic operating mode of the instrument.

Format: MODE,*type*

Arguments: type:
POWER (power meter)
INTEGR (integrator)
HARMON (harmonic analyser)
RMS (rms voltmeter)
LCR (LCR meter)
SCOPE (oscilloscope)
PHASEM (phase meter)

Reply: none

Example: MODE,LCR

Notes:

MSLAVE

MSLAVE

Function: Set master/slave mode

Description: Enables the instrument to synchronise with a second instrument to simultaneously measure up to 6 phases.

Format: MSLAVE,*type*

Arguments: type:
 DISABLE
 MASTER
 SLAVE

Reply: none

Example: MSLAVE,MASTER

Notes:

MULTIL**MULTIL**

Function: Selects data for multi string reply

Description: Selects data values across phases and functions that can be read in a single string.

Format: *MULTILOG,index,phase,function*

Arguments: index:
 0 clear all
 1-30 select data 1-30
 phase:
 1-3 phase 1-3
 4 sum
 5 neutral
 function:
 1-99 see appendix

Reply: none

Example: MULTIL,0
 MULTIL,1,1,2 (phase 1 Watts)
 MULTIL,2,2,2 (phase 2 watts)
 MULTIL,3,4,3 (sum VA)
 MULTIL?
 3 data values returned

Notes:

For further information and assistance with the Multilog application please go to page 2-102 where you will find an application guide to assist with this function

MULTIL?**MULTIL?**

Function:	Reads multi string reply	
Description:	Waits for data to be available then returns selected results.	
Format:	MULTILOG?	
Or:	MULTILOG, <i>lines?</i>	
Arguments:	Lines:	Integer
Reply:	Up to 60 data values as selected by the MULTILOG command in a single reply string OR Up to 60 data values as selected by the MULTILOG command in a single reply string, replying " <i>lines</i> " times.	
Example:	MULTIL,0	
	MULTIL,1,1,2	(phase 1 Watts)
	MULTIL,2,2,2	(phase 2 watts)
	MULTIL,3,4,3	(sum VA)
	MULTIL?	
	3 data values returned	
	MUTLIL,5?	
	Replies 5 times, each containing 3 data values	
Notes:	The MULTILOG, <i>lines?</i> command will reply each time a new data point is available.	

NEWLOC

NEWLOC

Function: Waits for new data then holds so that multiple commands can be used on the same data set.

Description: Reads multiple sets of data

Format: NEWLOC

Arguments: None

Reply: Data as per returned parameter query. ie from power, harmonics etc.

Example: NEWLOC;HARMON?SERIES;HPOWER?
Harmonic series and Power data returned

Notes: After the command the data will still be held so to release the lock send SUSPEND,OFF

NOISEF

NOISEF

Function: Sets the noise filter.

Description: Sets noise filter to value sent in string between 1KHz and 250KHz.

Format: NOISEF,[PHASEx],value,frequency

Arguments:

[PHASEx]:

Phase1

Phase2

Phase3

Value:

ON

OFF

frequency:

Between: 1000 – 250000

Reply: none

Example: NOISEF,PHASE1,ON,1500

Notes: Applies a digital filter for use in high noise environments. When in independent mode use [PHASEx] command to set noise filter on individual phases. [PHASESx] command is not required in any other wiring mode.

NOOVER

NOOVER

Function: Disable overranging

Description: Prevents an overrange error from blanking out results in manual ranging.

Format: NOOVER,*value*

Arguments: value:
 ON
 OFF

Reply: none

Example: NOOVER,ON

Notes: This can be useful when testing devices in a noisy environment. The range can be set to the correct range for the signal to be measured even if sporadic noise spikes would push it up on to the next range.

PFCONV

PFCONV

Function: Set power factor sign convention.

Description: Fundamental power factor is given a sign depending convention either:
negative if lagging current
negative if leading current

Format: PFCONV,*type*

Arguments: type:
NEGLAG
NEGLEA

Reply: none

Example: PFCONV,NEGLAG

Notes: An inductive load would have a lagging current, a capacitive load would have a leading current.
The sign given to VAr can be independently set: see VARCON

PHASEM

PHASEM

Function: Set phase meter mode.

Description: Select phase meter mode and reference.

Format: PHASE,*reference*

Arguments: reference:
 CH1 ratio = ch2/ch1
 CH2 ratio = ch1/ch2

Reply: none

Example: PHASEM,CH2

Notes:

PHASEM?**PHASEM?**

Function:	Phase meter query
Description:	Reads phase meter results. Sets phase meter mode if not already set. Waits for next unread data if available. Clears new data available bit read by DAV?
Format:	PHASEM? PHASEM, <i>phase?</i>
Arguments:	phase: PHASE1 PHASE2 PHASE3 PHASES?
Reply:	5 data values separated by commas freq,mag1,mag2,dB,phase
Example:	PHASEM,CH1 PHASEM,PHASE1? data returned
Notes:	The phase convention can be set to 0° to -360°, 0° to +360°, or +180° to -180° in the SYSTEM menu or using PHCONV command. PHASEM? without specifying the phase returns the appropriate single phase data.

PHCONV

PHCONV

Function: Set phase convention
Description: Set phase convention
Format: PHCONV,*convention*
Arguments: convention:
 180: -180 to +180
 -360: 0 to -360
 +360: 0 to +360
Reply: none
Example: PHCONV, -360
Notes: 0 to -360 degrees is usually used for power analysis applications

POWER

POWER

Function: Set up power analyser mode.

Description: Configure power analyser with sum current display type

Format: *POWER,sum type*

Arguments: sum type:
TOTAL
AVERAGE

Reply: none

Examples: POWER,TOTAL

Notes:

POWER?**POWER?**

Function: Read power analyser results

Description: Reads back latest power analyser results.
Sets power analyser mode.
Waits for next unread data if necessary.
Clears new data available status bit.

Format: *POWER,phase,results?*

Arguments: phase:
 PHASE1
 PHASE2
 PHASE3
 PHASES
 SUM
 NEUTRAL (current only)

results:
 WATTS
 VOLTAGE
 CURRENT
 VECTORS
 RMS
 WVA
 PH-PH

Reply: WATTS:
 freq,W,W.f,VA,VA.f,VA_r,VA_r.f,pf,pf.f,
 W_{dc},W_h

VOLTAGE or CURRENT:
 freq,rms,mag,dc,phase,pk,cf,mean,
 form factor,harm

VECTORS:
 freq,vmag1,vlag1,amag1,alag1.....

RMS:
 freq,vrms1,vdc1,arms1,adc1.....

WVA:
 freq,w1,vrms1,arms1,w2.....

PPA55xx communications manual

PH-PH:

freq,rms1,mag1,lag1,rms2...

Example: POWER,VECTORS?
data returned

Notes: POWER? without specifying the phase
returns the appropriate single phase data.
PHASES returns the data for all valid
phases 1-3.

PROGRA

PROGRA

Function: Access non volatile program stores.

Description: Recall, store or delete non-volatile program store.

Format: *PROGRA,function,number*

Arguments: function:
 RECALL
 STORE
 DELETE
 number
 0-100

Reply: none

Example: *PROGRA,RECALL,13*

Notes: Number 0 represents factory default, which can only be recalled.

PROGRA?

PROGRA?

Function: Identify current program.

Description: Reads the name of the last program to be loaded or recalled.

Format: PROGRA?

Arguments: none

Reply: text string

Example: PROGRA?
factory default

Notes:

RANGE**RANGE**

Function: Set channel ranging.

Description: Select minimum range and range control for a given input channel.

Format: *RANGE,channel,ranging,range*

Arguments: channel:
 CH1
 CH2
 ranging:
 AUTO
 UPAUTO
 MANUAL
 range:
 range number 1-9

Reply: none

Example: RANGE,CH2,MANUAL,4

Notes: CH1 sets the voltage range
 CH2 sets the current range
 Refer to the user manual for the range
 corresponding to each range number

RESOLU**RESOLU**

Function: Set the data resolution

Description: Data is returned in scientific format with exponent and mantissa. The resolution of the mantissa may be selected to be 5 digit (NORMAL) or 6 digit (HIGH) or 20 bit (BINARY).

Format: RESOLU,*format*

Arguments: format:
 NORMAL (5 digit mantissa)
 HIGH (6 digit mantissa)
 BINARY (compressed format)

Reply: none

Example: RESOLU,HIGH

Notes: Data format for NORMAL is:
 [-]1.2345E[-]00
 Data format for HIGH is:
 [-]1.23456E[-]00
 The sign of the mantissa and exponent are only sent if negative shown as [-] in the above examples
 BINARY format encodes each non-integer value in a proprietary 4 byte format for higher speed data transfer.

[Further notes on data format are included in section 1.4]

RESULT

RESULT

Function: Access non volatile results stores.
Description: Recall, store or delete non-volatile results.
Format: *RESULT,function,number*
Arguments: function:
 RECALL
 STORE
 DELETE
 number
 1-20
Reply: none
Example: RESULT,RECALL,13
Notes: There are 3 types of result: normal, harmonic and scope. Harmonic and scope results occupy 3 locations each.

RESULT?

RESULT?

Function: Identify used result stores.

Description: Reads a directory of the 20 non-volatile result locations.

Format: RESULT?

Arguments: none

Reply: 20 integers separated by commas

Example: RESULT?
0,0,1,3,-1,-1,0,2,-1,-1,0,0,0,0,0,0,0,0,0,0

Notes: 0 = empty
1 = normal result
2 = harmonic result
3 = scope result
-1 = continuation of previous

REZERO

REZERO

Function: Rezero front end

Description: Request the DSP to re-compensate for dc offset and compute a new autozero

Format: REZERO

Arguments: none

Reply: none

Example: REZERO

Notes:

SCALE

SCALE

Function: Set channel scale factor.

Description: Set a multiplying scale factor for a given input channel.

Format: *SCALE,channel,factor*

Arguments: channel:
 CH1
 CH2
 factor:
 multiplying scale factor

Reply: none

Example: SCALE,CH2,10

Notes: CH1 sets the scale for all voltage channels
 CH2 sets the scale for all current channels

SCOPE?**SCOPE?**

Function: Fetch raw scope data.

Description: Read back raw oscilloscope data.

Format: *SCOPE,channel?*
SCOPE,phase,channel?

Arguments: phase:
 PHASE1
 PHASE2
 PHASE3
 NEUTRA
 channel:
 VOLTAGE
 CURRENT

Reply: 252 signed integers:
 range
 trigger
 250 x data

Example: HOLD,ON
 SCOPE,PHASE1,VOLTAGE?
 read data
 SCOPE,PHASE2,VOLTAGE?
 read data
 SCOPE,PHASE3,VOLTAGE?
 read data
 HOLD,OFF

Notes:

SCREEN?

SCREEN?

Function: Read the screen data

Description: Returns a bit map of screen pixel display in ascii and hex format

Format: SCREEN?

Arguments: none

Reply: Multiple data bit values

Example: SCREEN?
data returned

Notes: SCREEN? response:

ASCII coded Hex
(2 characters for each byte)
240 lines of 40 bytes (each line represents one line of the display) preceded by #H
Each byte represents 8 dots where the lsb is the leftmost dot of the display
The bit is set for on and cleared for off

SETUP**SETUP**

Function:	Upload instrument set up
Description:	All the settings within the instrument may be read by SETUP?. The same settings may then be stored by ending the same data back to the instrument. As it sends all settings in a compressed format it is quicker than setting individual parameters.
Format:	SETUP,index,data
Arguments:	index: 0-15 data: ASCII hex as returned by SETUP?
Reply:	none
Example:	SETUP? Read 16 lines of data SETUP,00,data00 SETUP,01,data01 . . SETUP,15,data15
Notes:	The settings are only updated when the 16 th line has been received and the checksum has been verified.

SETUP?

SETUP?

Function: Read instrument set up

Description: All the settings within the instrument may be read by SETUP?. The same settings may then be stored by ending the same data back to the instrument. As it sends all settings in a compressed format it is quicker than setting individual parameters.

Format: SETUP?

Arguments: none

Reply: 16 lines of ASCII data

Example: SETUP?
Read 16 lines of data

Notes:

SHUNT

SHUNT

Function: Set channel shunt value

Description: Set the resistance factor of an external current shunt to be divided into the measured voltage for a given input channel.

Format: *SHUNT,channel,resistance*

Arguments: channel:
 CH1
 CH2
 resistance:
 shunt resistance in Ohms

Reply: none

Example: SHUNT,CH1,10

Notes: The shunt value is set for all current channels

SMOOTH**SMOOTH**

Function: Select the smoothing

Description: Sets the filter time constant and dynamic response.

Format: *SMOOTH,type,dynamics*

Arguments: type:
 NONE
 NORMAL
 SLOW
 dynamics:
 AUTO
 FIXED

Reply: none

Example: SMOOTH,NORMAL,FIXED
 SMOOTH,NONE

Notes: It is not necessary to send both parameters if it is only required to set the type. Both arguments must be sent to set the dynamics.
 FILTER is an alias for SMOOTH

SPEED

SPEED

Function: Sets the measurement speed

Description: Sets the minimum window size for the measurement.

Format: *SPEED,value,window*

Arguments: value:
VERY FAST
FAST
MEDIUM
SLOW
VSLOW
WINDOW

Reply: none

Example: SPEED,SLOW
SPEED,WINDOW,0.1

Notes: The window size argument is only needed for the SINDOW option

START

START

Function: Start datalog
Description: Initiate datalog data acquisition.
Format: START
Arguments: none
Reply: none
Example: DATALOG, RAM, 0.02
START
Notes:

STATUS?

STATUS?

Function: Read back channel ranging status.

Description: Read back condition of selected channel:
 range number (1-16)
 range text
 overflow/underflow status

Format: STATUS?
 or: STATUS,*channel*?
 STATUS?*channel*

Arguments: channel:
 CH1
 .
 .
 CH6

Reply: range number,range text,over/under/ok
 1-16
 range as per RANGE command
 OVER if overflow
 LOW if underflow
 OK if in range

Example: STATUS,CH1?
 6,300V,OK
 STATUS?
 OK

Notes:

STOP

STOP

Function: Stop datalog
Description: Stop datalog data acquisition.
Format: STOP
Arguments: none
Reply: none
Example: DATALOG, RAM, 0.02
START
wait for data values
STOP
read data values

Notes:

SUSPEN

SUSPEN

Function: Suspend data acquisition.

Description: Disable the data acquisition to maximise the communication speed.

Format: *SUSPEN,value*

Arguments: value:
ON
OFF

Reply: none

Example: FAST,ON
SUSPEN,ON
MULTILOG?
SUSPEN,OFF
FAST,OFF

Notes:

TAGREP

TAGREP

Function: Set up a reply tag

Description: Select a reply tag to identify the instrument in a multi-instrument environment

Format: TAGREP,*on/off*

Arguments: on/off:
ON
OFF

Reply: none

Example: TAGREP,ON
*ESR?
PPA5530:00635:1

Notes: When "tag reply" is turned on every reply string has a prefix of an identification string comprising the model and serial number

TEMPER

TEMPER

Function: Set up temperature measurement

Description: Set scaling and offset for a temperature sensor connected to the torque input (power transformer application mode)

Format: TEMPER,*type,scalefactor,offset*

Arguments: type:
 DISABLED
 CENTIG
 FARHEN
 scale:
 multiplying factor in degrees/Volt
 offset:
 additive zero in Volts

Reply: none

Example: TEMPER,CENTIG,5,-2
 sensor scaling = 5°C/V
 0V = 10°C

Notes:

TEMPER?

TEMPER?

Function: Read the temperature

Description: Returns the measured temperature from a sensor connected to the torque input

Format: TEMPER?

Arguments: none

Reply: single data value

Example: TEMPER?
data returned

Notes:

TORQSP

TORQSP

Function: Set up torque and speed measurement

Description: Set scaling for torque and speed measurements

Format: TORQSP,*type,torquescaling,speedscaling*
 TORQSP,OFFSET,*torqueoffset,speedoffset*

Arguments: type:
 DISABLED
 ANALOG
 PULSED
 OFFSET

Reply: none

Example: TORQSP,PULSED,10,50
 speed measured by pulse
 torque scaling = 10Nm/V
 50 pulses/revolution

Notes: If type = ANALOG then speed scaling is in rpm/V, if type = PULSED then speed scaling is pulses/rev
 Torque scaling is always Nm/V

TORQSP?

TORQSP?

Function: Read the mechanical power

Description: Returns measured mechanical data values

Format: TORQSP?

Arguments: none

Reply: 3 data values separated by commas:
power, torque, speed

Example: TORQSP?
data returned

Notes:

USER?

USER?

Function: Read the user data
Description: Returns up to 3 lines of user data
Format: USER?
Arguments: none
Reply: 3 lines of ASCII terminated by CR
Example: USER?
 Newtons4th Ltd
 R&D department
 KinetiQ #4

Notes:

VARCON

VARCON

Function: Set VAr sign convention.

Description: Fundamental VAr measurement is given a sign depending convention either:
negative if lagging current
negative if leading current

Format: VARCON,*type*

Arguments: type:
NEGLAG
NEGLEA

Reply: none

Example: VARCON,NEGLAG

Notes: An inductive load would have a lagging current, a capacitive load would have a leading current.
The sign given to power factor can be independently set: see PFCONV

VERSIO?

VERSIO?

Function: Read the instrument code versions.

Description: Returns an ASCII string with the details of the various parts of the instrument firmware.

Format: VERSIO?

Arguments: none

Reply: date code, type, cpu, dsp, fpga, boot type:
0 – normal (30A)
2 – low current version (10A)
4 – high current version (50A)

Examples: VERSION?
KQ1306,0,1.10,1.10,1.10,1.01

Notes: This data can be displayed on the screen by pressing SYSTEM then BACK

VRMS

VRMS

Function: Set up rms voltmeter.
Description: Set mode to rms voltmeter.
Format: VRMS
Arguments: none
Reply: none
Examples: VRMS
Notes: This has the same effect as MODE,VRMS

VRMS?**VRMS?**

Function: Read true rms voltmeter results

Description: Reads back latest voltmeter results.
Waits for next unread data if necessary.
Clears new data available status bit.

Format: *VRMS,phase,results?*

Arguments: results:
RMS
MEAN
SURGE
phase:
PHASE1
PHASE2
PHASE3
PHASES

Reply: RMS:
6 data values separated by commas
Vrms,Arms,Vdc,Adc,Vac,Aac
MEAN:
6 data values separated by commas
Vrms,Arms,Vmean,Amean,Vff,Aff
SURGE:
8 data values separated by commas
Vrms,Arms,Vpk,Apk,Vcf,Acf,
Vsurge1,Asurge

Example: VRMS,PHASE1,RMS?

Notes: VRMS? without specifying the phase returns the appropriate single phase data.

WIRING**WIRING**

Function: Select wiring mode.

Description: Set wiring mode for computation of SUM and neutral data.

Format: WIRING,*type*

Arguments: type:
SINGLE (single ph 1)
2PHASE (2 ph 2 wattmeter)
3PH2WA (3 ph 2 wattmeter)
3PH3WA (3 ph 3 wattmeter)
INDPH3 (3 ph 2 wattmeter + ph3)
PHASE1 (single ph 1)
PHASE2 (single ph 2)
PHASE3 (single ph 3)
INDEP (independent)

Reply: none

Examples: WIRING,PHASE2

Notes: WIRING,SINGLE is the same as WIRING,PHASE1

ZERO

ZERO

Function: Apply or remove the zero

Description: Applies or removes a zero function depending on the measurement mode (same as pressing ZERO key). Resets the integration data and timer if in power integration mode.

Format: ZERO
ZERO,DELETE

Arguments: none

Reply: none

Example: ZERO

Notes:

ZOOM**ZOOM**

Function: Sets the display zoom parameters.

Description: Sets the zoom level and data.

Format: *ZOOM,level,data1,data2,data3,data4*

Arguments: level:
 0 – normal
 1 – 2 line display (zoom level 1)
 2 – single line display (zoom level 2)
 3 – single line display (zoom level 3)
 data1:
 first data (zoom level 1)
 or data for single line (zoom level 2)
 data2-4:
 other data (zoom level 1)

data consists of line number for channel 1
 or line number + 128 for channel 2

Reply: None

Example: VRMS
 ZOOM,1,1,12 (level 1, ch1 rms, ch2 rms)

Notes: It is not necessary to send all the parameters, but whatever parameters are sent must be in the correct order.

ZOOM?

ZOOM?

Function: Read the display zoom parameters.

Description: Reads the zoom level and data.

Format: ZOOM?

Arguments:

Reply: 5 integers separated by commas:

level:

0 – normal

1 – 2-4 value display (zoom level 1)

2 – single line display (zoom level 2)

3 – single line display (zoom level 3)

data1-4:

zoom data

data consists of line number for channel 1
or line number + 128 for channel 2

Example:

ZOOM?

1,1,129,0,0 (level 1, ch1 rms, ch2 rms)

Notes:

Multilog Application Guide **Configuring the N4L PPA Power Analyzer for** **Data logging**

The Multilog (MULTIL) command provides an excellent method for data logging up to 64 parameters of information via one query command - MULTIL?

The instrument will return a comma-separated string which relates to the MULTIL,X,X,X setup commands previously entered by the relevant communication method. This enables the system to send one query and return up to 64 different parameters, from different phases in one response.

Step 1.

Reset "MULTILOG" using the **MULTIL,0** command

This will clear any previously entered Multilog parameters and ensure the instrument does not return unwanted results.

Step 2.

Set up the Multilog parameters

The format of the Multilog command is as follows

MULTILOG, Index, Phase, function

Index is the order in which the value is returned (Effectively allocating a "slot" for the parameter in the returned string)

Phase is the phase (PH1,PH2,PH3 etc) from which the result should be acquired.

Function is the parameter type (eg. Watts, VAr, Frequency etc) of the return.

PPA55xx communications manual

The Function ID is chosen from Appendix C which is a continually growing list due to firmware upgrades of the power analyzers at N4L, at present the PPA5500 has 87 possible functions:

Function	Measurement	Notes
1	frequency	
2	watts	
3	VA	
4	VAr	
5	power factor	
6	fundamental watts	
7	fundamental VA	
8	fundamental VAr	
9	fundamental PF	
10	harmonic watts	
11	harmonic watts %	
12	impedance	
13	resistance	

Example extract from the Multilog function list

Required Parameters

Order parameter to be returned within string	Phase (channel) of data returned	Parameter required
1	1	Frequency
2	1	Watts Phase 1
3	2	Watts Phase 2
4	3	Watts Phase 3
5	1	RMS Voltage Phase 1
6	2	RMS Voltage Phase 1
7	3	RMS Voltage Phase 1

MULTILOG Pattern

Command	Index	Phase	Function
MULTIL,	1	1	1
MULTIL,	2	1	2
MULTIL,	3	2	2
MULTIL,	4	3	2
MULTIL,	5	1	50
MULTIL,	6	2	50
MULTIL,	7	3	50

Command strings to sent, reference the above Multilog pattern;

MULTIL,0 // clears Multilog

MULTIL,1,1,1 // set Frequency as parameter 1

MULTIL,2,1,2 // set Phase 1 Watts as parameter 2

MULTIL,3,2,2 // set Phase 2 Watts as parameter 3

MULTIL,4,3,2 // set Phase 3 Watts as parameter 4

MULTIL,5,1,50 // set Phase 1 RMS Voltage as parameter 5

MULTIL,6,2,50 // set Phase 2 RMS Voltage as parameter 6

MULTIL,7,3,50 // set Phase 3 RMS Voltage as parameter 7

Step 3.

Send Multil query and read return string.

MULTIL? // returns a comma separated string as

Example return string:

5.0000E1, 2.4500E2, 2.4320E2, 2.5421E2, 1.0232E3, 1.0152E3, 1.0546E3
↑ ↑ ↑ ↑ ↑ ↑ ↑
Frequency PH1 Watts PH2 Watts PH3 Watts PH1 RMS Volt PH2 RMS Volt PH3 RMS Volt

Appendix – command summary

COMMAND SUMMARY

PPA55xx communications manual

command format	reply format
*CLS	
*ESE,value	
*ESE?	single integer data value
*ESR?	single integer data value
*IDN?	company,product,serial no,version
*OPC?	0 or 1
*RST	
*SRE,value	single integer data value
*SRE?	
*STB?	single integer data value
*TRG	
*TST?	single integer data value
*WAI	
ABORT	
ALARM,latch,sounder	
ALARM?	single integer data value
ALARME,value	
ALARME?	single integer data value
ALARM1,type,data,high,low	
ALARM2,type,data,high,low	
APPLIC,type,setting	
BANDWI,phase,type	
BEEP	
BLANKI,on/off,threshold	
CALVER,string	
CALVER?	String
CAPTUR?	String
CONFIG,parameter,data	
CONFIG,parameter?	single integer or real data value
COUPLI,phase,coupling	
DATALO,func,interval,speed	
DATALO,LINES?	single integer
DATALO,0?	index,time,data... one record per line
DATALO,start,records?	index,time,data... one record per line
DAV?	single integer data value
DAVER,value	
DAVER?	single integer data value
DISPLAY,page	
DISPLAY?	multiple real data values
EFFICI,type	
EFFICI?	total efficiency, fundamental efficiency

PPA55xx communications manual

FAST,on/off	
FQLOCK,on/off	
FQREF,phase,channel	
FREQFI,on/off,filter	
FREQUE,frequency	
FSD?	Single or multiple real data values
HARMON,para,h,hmax	
HARMON,phase?	freq,mag1,mag2,hmag1,hmag2,h1,h2, thd1,thd2,hphase1,hphase2
Or	
HARMON,phase,SERIES?	mag,%, x n harmonics
Or	
HOLD,on/off	
INPUT,channel,type	
INTEGR,type,display	
INTEGR,RUNTIM,hours,mins	
INTEGR,phase?	Time,Wh,Wh.f, Varh,Varh.f,Vah,Vah.f, pf,pf.f,Vav,Vav.fAh,Ah.f
KEYBOA,value	
LCR,conditions,param,head	
LCR,phase?	Freq,mag1,mag2,impedance,phase,R, L,C (series),R,L,C (parallel),tan δ ,Q
LOWFRE,on/off	
MODE,type	
MSLAVE,type	
MULTILOG,index,phase,func	
MULTILOG?	1-30 floats as selected
PFCNV,convention	
PHASEM,ratio	
PHASEM,phase?	Freq,mag1,mag2,dB,phase
PHCONV,convention	
POWER,sum A	
POWER,PHASE,WATTS?	Freq,W,W.f, VA,VA.f,Var,Var.f,pf,pf.f, Wdc,W.h
POWER,PHASE,VOLTAGE?	Freq,rms,mag,dc, ϕ ,peak,cf,mean,ff, harmonic
POWER,PHASE,CURRENT?	Freq,rms,mag,dc, ϕ ,peak,cf,mean,ff, harmonic
POWER,PH-PH?	Freq,rms1,mag1, ϕ 1,rms2,mag2, ϕ 2, rms3,mag3, ϕ 3
POWER,RMS?	Freq,vrms1,vdc1,arms1,adc1,vrms2, vdc2,arms2,adc2,vrms3,vdc3, arms3, adc3

PPA55xx communications manual

POWER,VECTORS?	Freq,mag1, ϕ 1,mag2, ϕ 2,mag3, ϕ 3, mag4, ϕ 4,mag5, ϕ 5,mag6, ϕ 6
POWER,WVA?	Freq,w1,vrms1,arms1,w2,vrms2, arms2,w3,vrms3,arms3
PROGRAM,function,number PROGRAM?	CR terminated text string
RANGE,ch,ranging,range RESOLU.format	
RESULT,function,number RESULT	multiple integers
REZERO	
SCALE,channel,factor SCALE,channel?	Single real data value
SCOPE,PHASE,v/a?	Range, trigger, 250 signed integer values
SHUNT,channel,resistance SHUNT,channel?	Single real data value
SMOOTH,type,dynamics	
SPEED,value>window	
START	
STATUS,channel?	Range number,range text,over/low/ok
STOP	
STREAM,enable>window STREAM,disable	
STREAM?	Data, data, data, data, data,
SUSPEN,on/off	
TAGREP,on/off	
TEMPER,type,scale,offset TEMPER?	single real data value
TORQSP,type,tscale,sscale TORQSP,OFFSET,toff,soff TORQSP?	mechanical power, torque, speed
USER?	3 CR terminated text strings
VARCON,convention	
VERSION?	datecode,cpu,dsp,fpga,boot
VRMS	
VRMS,PHASE,RMS?	rms1,rms2,dc1,dc2,ac1,ac2
VRMS,PHASE,MEAN?	rms1,rms2,mean1,mean2,ff1,ff2
VRMS,PHASE,SURGE?	pk1,pk2,cf1,cf2,surge1,surge2
WIRING,configuration	
ZERO	
ZERO,DELETE	
ZOOM,level,d1,d2,d3,d4 ZOOM?	level,d1,d2,d3,d4

PPA55xx communications manual

calibration commands

CALAPP	
CALCOM,freq	
CALFIL,index,value	
CALFIL?	Six real data values
CALFRQ,index,freq	
CALFRQ?	Seven real data values
CALIBR,index,value,inputs	
CALIBR?	Single integer data value
CALIDS,string	
CALIDS?	String
CALJIG,value	
CALMOD,value	
CALPHA,index,inputs	
CALRES	
CALSAV,password	
CALSYS,index,value,inputs	
CALSNO,serial number	
CALSTR,string	
CALSTR?	String
CALTQS,index,value	
CALTQS?	Four real data values
CALVER,string	
CALVER?	String

PPA55xx communications manual

Appendix B – Configurable parameters

All parameters can be accessed using the CONFIG command:

<i>number</i>	Function	<i>parameter</i>
1	Operating mode, (sets Main Mode)	0=RMS Voltmeter 1=Phase Meter 2=Power Analyser 3=Impedance Analyser 4=Power Integrator 5=Harmonic Analyser 7=Oscilloscope
2	Resolution, (remote options – digit resolution)	0=Normal 1=High 2=Binary
3	Master/slave, (Aux control)	0=Disabled 1=Master 2=Slave
4	Autozero manual or auto, (System options)	0=Auto 1=Manual
6	Phase convention, (System options)	0=-180° to +180° 1=0° to -360° 3=0° to +360°
7	Frequency lock on/off, (Acquisition advance options)	0=Off 1=On
8	Graph, (System options)	0=Dots

PPA55xx communications manual

1=Lines

- 9 Keyboard beep on/off, (System options)
 0=Off
 1=On
- 10 Ignore overload,(Acquisition advance options)
 0=Off
 1=On
- 11 Low frequency mode, (Acquisition control)
 0=Off
 1=On
- 12 Window size, (Acquisition control, speed-window)
 0=ms
 1=Sec's
- 13 Speed, (Acquisition control or Phase meter)
 0=Very Slow
 1=Slow
 2=Medium
 3=Fast
 4=Very Fast
 5=Window
- 14 Smoothing (Acquisition Control or Phase Meter)
 0=Normal
 1=Slow
 2=None
- 15 Smoothing Response (Acquisition Control or Phase meter)
 0=Auto reset
 1=Fixed time
- 16 Baud rate, (Remote options , RS232)
 0=38400
 1=19200
 2=9600
 3=1200
- 18 LAN IP address nibble 3, (Remote options - LAN - enter figure as required)
- 19 LAN IP address nibble 2, (Remote options - LAN - enter figure as required)
- 20 LAN IP address nibble 1, (Remote options - LAN - enter figure as required)

PPA55xx communications manual

- 21 LAN IP address nibble 0, (Remote options - LAN - enter figure as required)
- 22 Independent ranging, (System options)
0=Disabled
1=Enabled
- 24 Enable channel 1, (Range - voltage input)
0=Internal
3=External Attenuator
- 25 Enable channel 2, (Range - current input)
0=Internal
2=External Shunt
- 26 Input range channel 1, (Range - minimum range voltage)
0=300mv
1=1v
2=3v
3=10v
4=30v
5=100v
6=300v
7=1kV
8=3KV
- 27 Input range channel 2, (Range - minimum range current)
0=30ma
1=100ma
2=300ma
3=1A
4=3A
5=10A
6=30A
7=100
8=300A
- 28 Input ranging channel 1, (Range - autoranging voltage)
0=Full Autorange
1=Range up only
2=Manual
- 29 Input ranging channel 2, (Range - autoranging current)
0= Full Autorange
1=Range up only

PPA55xx communications manual

2=Manual

- 30 **Coupling, (Coupling)**
 - 0=ac+dc
 - 1=ac
 - 2=dc

- 31 **Bandwidth, (Coupling - bandwidth)**
 - 0=Wide (dc-2MHz)
 - 1=Low (dc-200KHz)
 - 2=dc (dc-5Hz)

- 32 **Scale factor channel 1 voltage, (Ranging - Enter figures as required)**

- 33 **Scale factor channel 2 current, (Ranging - Enter figures as required)**

- 34 **External attenuator channel 1, (Ranging - voltage input - attenuator ratio - Enter figures as required)**

- 35 **External shunt channel 2, (Ranging - current input - resistance value- Enter figures as required)**

- 38 **Frequency reference voltage/current, (Acquisition control)**
 - 0=Voltage
 - 1=Current
 - 2=Speed
 - 3=ac line

- 40 **Frequency reference phase, (Acquisition control)**
 - 0=Phase 1
 - 1=Phase 2
 - 2=Phase 3

PPA55xx communications manual

- 41 Display page, (Main display)
 0=Phase 1 page
 1=Phase 2 page
 2=Phase 3 page
 3=Sum page
 4=Phase 1,2 &3 page
 5=Phase 1,2 & 3 fundamentals page
 6=NEU page
- 42 Zoom level, (Main display)
 0=Zoom -
 1=Zoom +
 2=second Zoom +
- 43 Function zoomed on 1, (Main display)
 0=Voltage, Current & Frequency
 1=Watts, Current, Voltage & Frequency
 2= VA, Current, Voltage & Frequency
 3= VAr, Current, Voltage & Frequency
 4= pf, Current, Voltage & Frequency
- 44 Function zoomed on 2, (Main display)
 0=Current & Frequency
 1= Watts, Current & Frequency
 2= VA, Current & Frequency
 3= VAr, Current & Frequency
 4= pf, Current & Frequency
 5= Current, Voltage & Frequency
- 45 Function zoomed on 3, (Main display)
 0= Watts & Frequency
 2= Watts, VA & Frequency
 3= Watts, VAr & Frequency
 4= Watts, pf & Frequency
 5= Watts, Voltage & Frequency
 6= Watts, Current & Frequency

PPA55xx communications manual

- 46 **Function zoomed on 4,** (Main display)
 0= Watts & VA
 3= Watts, VA & VAr
 4= Watts, VA & pf
 5= Watts, VA & Voltage
 6= Watts, VA & Current
 7= Watts, VA & Frequency
 8= Watts, VA & Harmonic
 9= Watts, VA & dc watts
 10= Watts, VA & V Ph-Ph
- 47 **Datalog display type,** (Datalog display information mode)
 0=Real Time
 1=Table
 2=Graph
- 48 **Manual frequency,** (Acquisition advance options – frequency lock on)
 0=Frequency in μ hz
 1=Frequency in Hz
- 49 **DFT selectivity,** (Acquisition advance options)
 0=Normal
 1=Narrow
- 50 **Program 1-6 direct load,** (System options)
 0=Disabled
 1=Enabled
- 51 **Language,** (System options)
 0=English
 1=Other language if installed
- 52 **Frequency filter,** (Acquisition control)
 0=Disabled
 1=Enabled
- 53 **Phase reference,** (Acquisition control)
 0=Voltage
 1=Current
- 54 **Datalog Zoom1,** (Datalog-RAM)
 0=Enabled
 1=Disabled

PPA55xx communications manual

- 55 Datalog Zoom2, (Datalog-RAM)
 0=Enabled
 1=Disabled
- 56 Datalog Zoom3, (Datalog-RAM)
 0=Enabled
 1=Disabled
- 57 Datalog Zoom4, (Datalog-RAM)
 0=Enabled
 1=Disabled
- 58 Datalog memory type, (Datalog)
 0=Disabled
 1=RAM
- 59 Datalog Interval, (Datalog) (Enter interval time figure in seconds)
- 60 Datalog graph, (Datalog-RAM)
 0=Together
 1=Seperate
- 61 Formula, (Maths)
 0=Disabled
 1=(term1 + term2/term3 + term4)
 2=(term1 + term2) x term3/term4
 3=term1 x term2/(term3 + term4)
- 62 Argument term 1
 0=Disabled
 1=Constant
 2=Voltage
 3=Current
 4=Torque
 5=Speed
- 63 Sub argument term 1, (For voltage and current arguments only)
 0=rms
 1=dc
 2=ac
 3=Fundamental
 4=Peak

PPA55xx communications manual

- 5=Mean
- 6= Ph-Ph rms
- 7=Ph-Ph mag

- 64 Term 1 coefficient, (Enter value)

- 65 Argument term 2,
 - 0=Disabled
 - 1=Constant
 - 2=Voltage
 - 3=Current
 - 4=Torque
 - 5=Speed

- 66 Sub argument term 2, (For voltage and current arguments only)
 - 0=rms
 - 1=dc
 - 2=ac
 - 3=Fundamental
 - 4=Peak
 - 5=Mean
 - 6= Ph-Ph rms
 - 7=Ph-Ph mag

- 67 Term 2 coefficient, (Enter value)

- 70 application mode,
 - 0=Normal
 - 1=PWM motor Drive
 - 2=Lighting ballast
 - 3=Inrush current
 - 4=Transformer mode
 - 5=Standby power

- 71 Frequency filter, (Application options mode - PWM Motor Drive)
 - 0=4KHz
 - 1=1KHz
 - 2=250Hz

- 72 Frequency tracking speed, (Application options mode - Lighting Ballast)
 - 0=Fixed time
 - 1=Fast
 - 2=Medium
 - 3=Slow

PPA55xx communications manual

- 73 Low frequency, (Application options mode - PWM Motor Drive)
 0=Off
 1=On
- 74 Argument term 3
 0=Disabled
 1=Constant
 2=Voltage
 3=Current
 4=Torque
 5=Speed
- 75 Sub argument term 3, (For voltage and current arguments only)
 0=rms
 1=dc
 2=ac
 3=Fundamental
 4=Peak
 5=Mean
 6= Ph-Ph rms
 7=Ph-Ph mag
- 76 Term 3 coefficient, (Enter value)
- 77 Argument term 4
 0=Disabled
 1=Constant
 2=Voltage
 3=Current
 4=Torque
 5=Speed
- 78 Sub argument term 4, (For voltage and current arguments only)
 0=rms
 1=dc
 2=ac
 3=Fundamental
 4=Peak
 5=Mean
 6= Ph-Ph rms
 7=Ph-Ph mag
- 79 Term 4 coefficient, (Enter value)

PPA55xx communications manual

- 80 **Temperature,** (Application-Transformer mode)
 0=Disabled
 1=Enabled °C
 2=Enabled °F
- 81 **Sum watts,** (Auxiliary-Master)
 0=Master
 1=Master + Slave
- 82 **Wiring configuration,** (Acquisition control)
 0=Single phase 1
 1=2 phase 2 wattmeter
 2=3 phase 2 wattmeter
 3=3 phase 3 wattmeter
 4=Single phase 2
 5=Single phase 3
 6=3 phase 2 wattmeter + PH3
 7=Independent
- 83 **Integration,** (Power analyzer - Power integrator)
 0=Signed
 1=Magnitude
- 84 **Torque + speed,** (Application options – PWM motor drive)
 0=Disabled
 1=Analogue speed
 2=Pulsed speed
- 85 **Torque scaling Nm/V,** (Applications – PWM motor drive) (Also transformer
 scale factor Deg/v)(Enter Nm/v value)
- 86 **Speed scaling Hz/V,**(Applications – PWM motor drive)(Enter rpm/v value)
- 87 **Pulses per revolution,**(Applications–PWM motor drive)(Enter pulses/rev value)
- 88 **Integration display,** (Mode - Power integrator)
 0=Total
 1=Average
- 89 **Sum current average,** (Power analyzer)
 0=Total
 1=Average
- 90 **Phase 3 reference,** (Acquisition control – 3 phase 2 wattmeter + PH3)

PPA55xx communications manual

- 0=Voltage
 - 1=Current
 - 2=ac line
 - 3=Phase 1 & 2
- 91 Power factor sign, (Power analyzer)
- 0=Negative lagging
 - 1=Negative leading
- 92 VAr sign, (Power analyzer)
- 0= Negative lagging
 - 1=Negative leading
- 93 Efficiency computation, (Power analyzer)
- 0=Disabled
 - 1=Phase 1 / Phase 2
 - 2=Phase 2 / Phase 1
 - 3=Slave/Master
 - 4=Master/Slave
 - 5=Mechanical/Sum
 - 6=Sum/Mechanical
 - 7=Phase 3/Sum
 - 8=Sum/Phase 3
- 94 Range lock across phases, (Range – when acquisition is using 3 phases)
- 0=Disabled
 - 1=Enabled
- 95 Torque offset, (Applications–PWM motor drive)(Also transformer mode)(Enter Nm offset value)
- 96 Speed offset, (Application options mode – PWM motor drive – rpm offset value)
- 99 Computation mode, (Harmonic analyzer)
- 0=Difference formula
 - 1=Harmonic series
 - 2=TIF
 - 3=THF
 - 4=TRD
 - 5=TDD
 - 6=Series harmonic phase
- 100 Selected harmonic, (Harmonic analyzer - figure = harmonic required)

PPA55xx communications manual

- 101 Harmonic series up to, (Harmonic analyzer - figure = harmonic max)
- 102 Voltage bargraph scale, (Harmonic analyzer - figure = % required)
- 103 Current rating (TRD), (Harmonic analyzer - TRD mode - enter figure)
- 104 Current bargraph scale, (Harmonic analyzer - figure = % required)
- 106 Timebase, (Scope - Enter figure/div)
- 107 trigger level, (Scope - Enter figure/div)
- 108 Pretrigger, (Scope)
0=None
1=25%
2=50%
3=75%
- 109 trigger polarity, (Scope)
0=Rising edge
1=Falling edge
- 110 trigger Mode, (Scope)
0=Auto
1=Normal
2=Single shot
- 111 trigger reference, (Scope)
0=Voltage
1=Current
- 112 trigger phase, (Scope)
0=Phase 1
1=Phase 2
2=Phase 3
- 113 cursors enable, (Scope)
0=Off
1=On
- 114 trigger HF reject, (Scope)
0=Off
1=On

PPA55xx communications manual

- 115 Trace, (Scope)
0=Dual
1=Voltage
2=Current
- 119 zoom 2 high resolution, (System)
0=Disabled
1=Enabled
- 120 Brightness, (System)
0=Low
1=High
- 121 Display, (System)
0=Colour
1=White on black
2=Black on white
- 122 Auxiliary device, (Aux control)
0=None
6=PCIS
- 128 Switch phase offset, (Aux control – PCIS device)
0=0°
1=45°
2=90°
3=135°
4=180°
5=225°
6=270°
7=315°
- 129 Switch on cycles, (Aux control – PCIS device)
0=Single cycle
1=Continuous
2=Half cycle
- 130 Gear ratio, (Aux control – frequency reference – speed - Enter ratio value)
- 131 2 Wattmeter sum computation, (Power Analyser)(select in acquisition wiring-2 phase 2 wattmeter)
0=Low distortion
1=High Distortion

PPA55xx communications manual

- 132 Integrator-run time (Hours), (Mode - Power integrator - enter figure)
- 133 Integrator-Run time (mins), (Mode - Power integrator - enter figure)
- 134 Ph - Ph Measurement, (Power analyser)
0=Rms
1=Mean
- 135 Difference THD, (Power analyser)
0=Disabled
1=Enabled
- 137 Parameter, (Impedance analyzer)
0=Auto
1=Capacitance
2=Inductance
3=Impedance
- 138 Measurement, (Impedance analyzer)
0=Series
1=Parallel
- 139 Phase offset, (Impedance analyzer - Enter figures)
- 144 Rectified mean, (rms voltmeter)
0=Absolute
1=Normalised
- 148 dB offset, (Phase meter - Enter figures)
- 150 Computation, (Phase meter)
0=ch2/ch1
1=ch1/ch2
- 152 RS232 printer enable, (Remote options)
0=Disabled
1=Enabled
- 153 IEEE address, (Remote options - GPIB mode - enter address figures)
- 154 Interface, (Remote options)
0=RS232

- 1=USB
- 2=LAN
- 3=GPIB

- 155 Recall with program, (Remote options)
0=Off
1=On

Alarm functions

- 156 Alarm 1 data, (Alarm options)
0=Zoom1
1=Zoom 2
2=Zoom3
3=Zoom 4

- 157 Alarm 1 type, (Alarm options)
0=Disabled
1=Linear
2=Alarm if high
3=Alarm if low
4=Outside window
5=Inside window

- 158 Alarm 1 high threshold, (Alarm options – alarm if high – enter figure)

- 159 Alarm 1 low threshold, (Alarm options – alarm if low – enter figure)

- 160 Alarm latch, (Alarm options – alarm if high)
0=Off
1=On

- 161 Alarm sounder, (Alarm options – alarm if high)
0=Enabled
1=Disabled

- 162 Analog output, (Alarm options – alarm if high)
0=Disabled
1=Zoom 1
2=Zoom 2
3=Zoom 3
4=Zoom 4
5=Manual

PPA55xx communications manual

- 164 Analog zero, (Alarm options – enter figure)
- 165 Analog full scale, (Alarm options – enter figure)
- 167 Alarm 2 data, (Alarm options)
0=Zoom 1
1=Zoom 2
2=Zoom 3
3=Zoom 4
- 168 Alarm 2 type, (Alarm options)
0=Disabled
1=Linear
2=Alarm if high
3=Alarm if low
4=Outside window
5=Inside window
- 169 Alarm 2 high threshold, (Alarm options – alarm if high – enter figure)
- 170 Alarm 2 low threshold, (Alarm options – alarm if low – enter figure)
- 171 Sync on alarm, (Alarm options – alarm if high)
0=Disabled
3=Enabled
- 176 Enable channel 3, (Range–voltage input)(Sys - independent ranging enabled)
0=Internal
3=External attenuator
- 177 Enable channel 4, (Range - current input)(Sys independent ranging enabled)
0=Internal
2=External shunt
- 178 Input range channel 3, (Range - minimum range voltage) (Sys independent ranging enabled)
0=300mv
1=1v
2=3v
3=10v
4=30v
5=100v
6=300v
7=1kV

PPA55xx communications manual

8=3KV

- 179 Input range channel 4, (Range - minimum range current) (Sys independent ranging enabled)
 0=30ma
 1=100ma
 2=300ma
 3=1A
 4=3A
 5=10A
 6=30A
 7=100
 8=300A
- 180 Input ranging channel 3, (Range - autoranging voltage) (Sys independent ranging enabled)
 0=Full Autorange
 1=Range up only
 2=Manual
- 181 Input ranging channel 4, (Range - autoranging current) (Sys independent ranging enabled)
 0= Full Autorange
 1=Range up only
 2=Manual
- 182 Coupling phase 2, (Coupling) (Sys independent ranging enabled)
 0=ac +dc
 1=ac
 2=dc
- 183 Bandwidth phase 2,(Coupling - bandwidth) (Sys independent ranging enabled)
 0=Wide (dc-2MHz)
 1=Low (dc-200KHz)
 2=dc (dc-5Hz)
- 184 Scale factor channel 3 voltage, (Ranging - Enter figures as required)(Sys independent ranging enabled)
- 185 Scale factor channel 4 current, (Ranging - Enter figures as required) (Sys independent ranging enabled)
- 186 External attenuator channel 3,(Ranging - voltage input - attenuator ratio Enter figures as required)(Sys independent ranging enabled)

PPA55xx communications manual

- 187 External shunt channel 4, (Ranging – current input – resistance value Enter figures as required) (Sys independent ranging enabled)
- 200 Enable channel 5, (Range – voltage input) (Sys independent ranging enabled)
0=Internal
3=External attenuator
- 201 Enable channel 6, (Range – current input) (Sys independent ranging enabled)
0=Internal
2=External shunt
- 202 Input range channel 5, (Range – minimum range voltage)
0=300mv
1=1v
2=3v
3=10v
4=30v
5=100v
6=300v
7=1kV
8=3KV
- 203 Input range channel 6, (Range – minimum range current) (Sys independent ranging enabled)
0=30ma
1=100ma
2=300ma
3=1A
4=3A
5=10A
6=30A
7=100
8=300A
- 204 Input ranging channel 5, (Range – autoranging voltage) (Sys independent ranging enabled)
0=Full Autorange
1=Range up only
2=Manual
- 205 Input ranging channel 6, (Range – autoranging current) (Sys independent ranging enabled)

PPA55xx communications manual

- 0= Full Autorange
1=Range up only
2=Manual
- 206 Coupling phase 3, (Coupling) (Sys independent ranging enabled)
0=ac +dc
1=ac
2=dc
- 207 Bandwidth phase 3,(Coupling - bandwidth) (Sys independent ranging enabled)
0=Wide (dc-2MHz)
1=Low (dc-200KHz)
2=dc (dc-5Hz)
- 208 Scale factor channel 5 voltage,(Ranging - Enter figures as required) (Sys independent ranging enabled)
- 209 Scale factor channel 6 current, (Ranging - Enter figures as required) (Sys independent ranging enabled)
- 210 External attenuator channel 5,(Ranging - voltage input - attenuator ratio as required) (Sys independent ranging enabled)
- 211 External shunt channel 6, (Ranging - current input - resistance value as required) (Sys independent ranging enabled)
- 217 Memory, (Program)
0=Internal
1=USB Memory stick
- 218 Data, (Program)
0=Program
1=Results
2=Datalog
- 219 Action, (Program)
0=Recall
1=Store
2=Delete
- 220 Location, (Program - Enter figures as required)
- 225 Set clock hours, (System - Enter figures as required)

PPA55xx communications manual

- 226 Set clock minutes, (System – Enter figures as required)
- 227 Set clock Seconds, (System – Enter figures as required)
- 228 Set date day, (System – Enter figures as required)
- 229 Set date month, (System – Enter figures as required)
- 225 Set date year, (System – Enter figures as required)

PPA55xx communications manual

Appendix C – MULTILOG parameters

function	measurement	notes
1	frequency	
2	watts	
3	VA	
4	VAr	
5	power factor	
6	fundamental watts	
7	fundamental VA	
8	fundamental VAr	
9	fundamental PF	
10	harmonic watts	
11	harmonic watts %	
12	impedance	
13	resistance	
14	reactance	
15	impedance phase	
16	efficiency	
17	fundamental efficiency	
18	maths	
19	integrated watts	integrator mode
20	integrated VA	integrator mode
21	integrated VAr	integrator mode
22	integrated rms current	integrator mode
23	average power factor	integrator mode
24	integrated fundamental watts	integrator mode
25	integrated fundamental VA	integrator mode
26	integrated fundamental VAr	integrator mode
27	integrated fundamental current	integrator mode
28	average fundamental power factor	integrator mode
29	average integrated watts	integrator mode
30	average integrated VA	integrator mode
31	average integrated VAr	integrator mode
32	average integrated fundamental watts	integrator mode
33	average integrated fundamental VA	integrator mode
34	average integrated fundamental VAr	integrator mode
35	average rms voltage	integrator mode
36	average fundamental voltage	integrator mode
37	Standby mode frequency	
38	DC watts	

PPA55xx communications manual

39	average rms current	integrator mode
40	average fundamental current	integrator mode
41	delta watts	
42	fundamental delta watts	
43	elapsed time	integrator mode
44	reserved for future expansion	
45	reserved for future expansion	
46	reserved for future expansion	
47	reserved for future expansion	
48	reserved for future expansion	
49	reserved for future expansion	
50	rms voltage	
51	rms current	
52	fundamental voltage	
53	fundamental current	
54	voltage phase	
55	current phase	
56	harmonic voltage	
57	harmonic current	
58	dc voltage	
59	dc current	
60	ac voltage	
61	ac current	
62	peak voltage	
63	peak current	
64	voltage crest factor	
65	current crest factor	
66	rectified mean voltage	
67	rectified mean current	
68	voltage form factor	
69	current form factor	
70	voltage harmonic	
71	current harmonic	
72	voltage harmonic percentage	
73	current harmonic percentage	
74	voltage thd	harmonic mode
75	current thd	harmonic mode
76	voltage tif	harmonic mode
77	current tif	harmonic mode
78	phase to phase rms voltage	
79	phase to phase fundamental voltage	
80	phase to phase voltage phase angle	
81	phase to phase rms voltage	

PPA55xx communications manual

82	voltage surge	
83	current surge	
84	voltage rms deviation	transformer mode
85	voltage fundamental deviation	transformer mode
86	voltage phase deviation	transformer mode
87-99	reserved for future expansion	

PPA55xx communications manual

Some special functions:

measurement	phase	function
mechanical speed in Hz	neutral	dc voltage
mechanical speed in rpm	neutral	ac voltage
torque in Nm	neutral	rms voltage
mechanical power	neutral	watts

Phase selection:

- 1 = phase 1
- 2 = phase 2
- 3 = phase 3
- 4 = sum
- 5 = neutral

Newton4th Ltd. contact details

Please direct all queries or comments regarding the PPA25xx instruments or this manual to:

Newton4th Ltd.
30 Loughborough Rd.
Mountsorrel
LOUGHBOROUGH
LE12 7AT
United Kingdom

Tel: (0116) 230 1066 international +44 116 230 1066
Fax: (0116) 230 1061 international +44 116 230 1061

At Newton4th Ltd. we have a policy of continuous product improvement and are always keen to hear comments, whether favourable or unfavourable, from users of our products. Please telephone, fax, write or e-mail with your comments.

USED4TEST

Телефон: +7 (499) 685-7744

used@used4test.ru

www.used4test.ru